



**Figure 1**

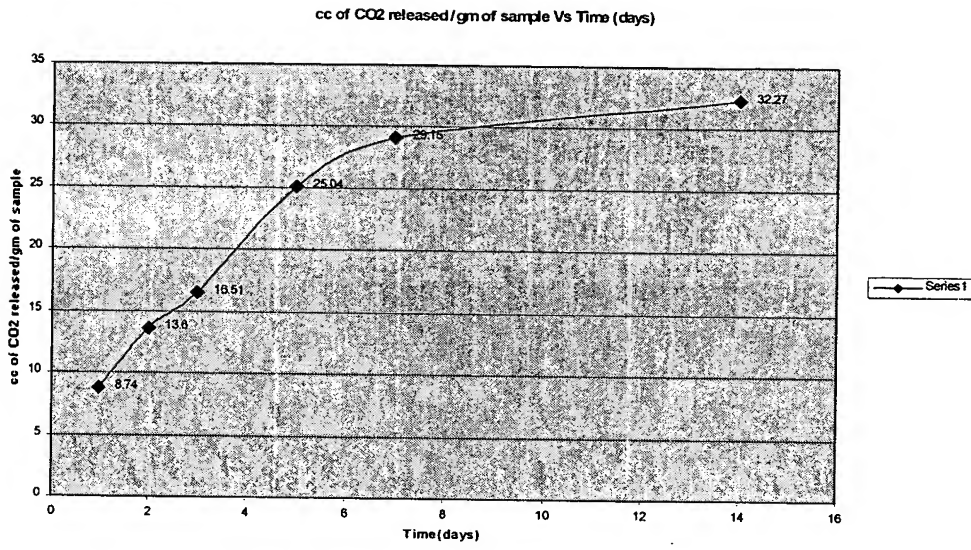

105731 666007


**Figure 2**

Leakproof vials (control samples)  
% of oxygen inside vials Vs Time (Days)

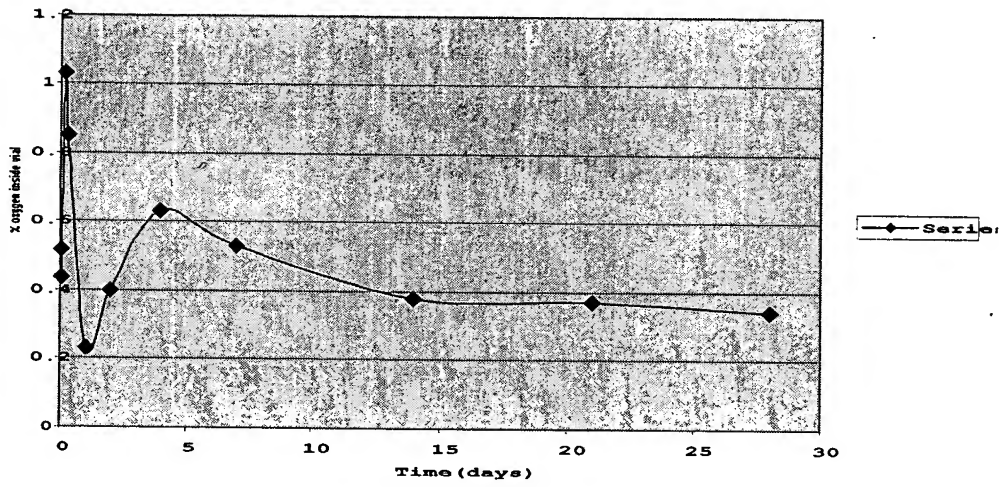

10033973.124901

# CO2 release by the film X1147 (Sodium bicarbonate with malic acid)

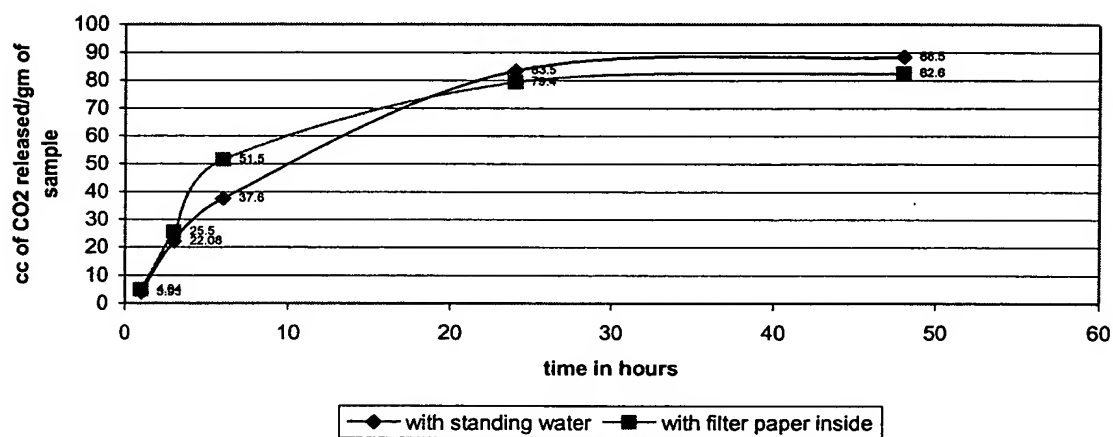

**FIGURE 3**